
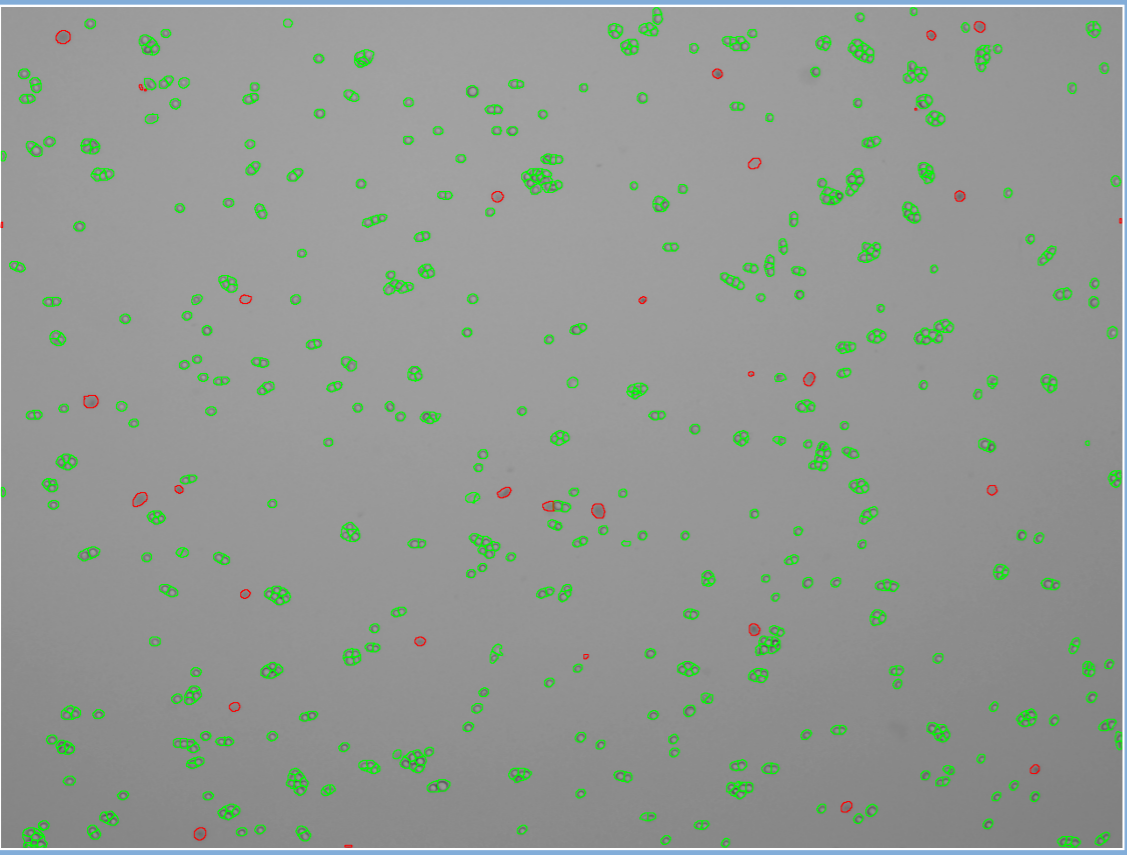


Countess II Live/Dead Report

File name: 20190523 hct chop 1000 rep 3_R.pdf
Date: 05.24.2019 08:19:30 AM

Results:

Concentration		
Total		4.14 x 10 ⁶ /mL
Live	95%	3.95 x 10 ⁶ /mL
Dead	5%	1.88 x 10 ⁵ /mL

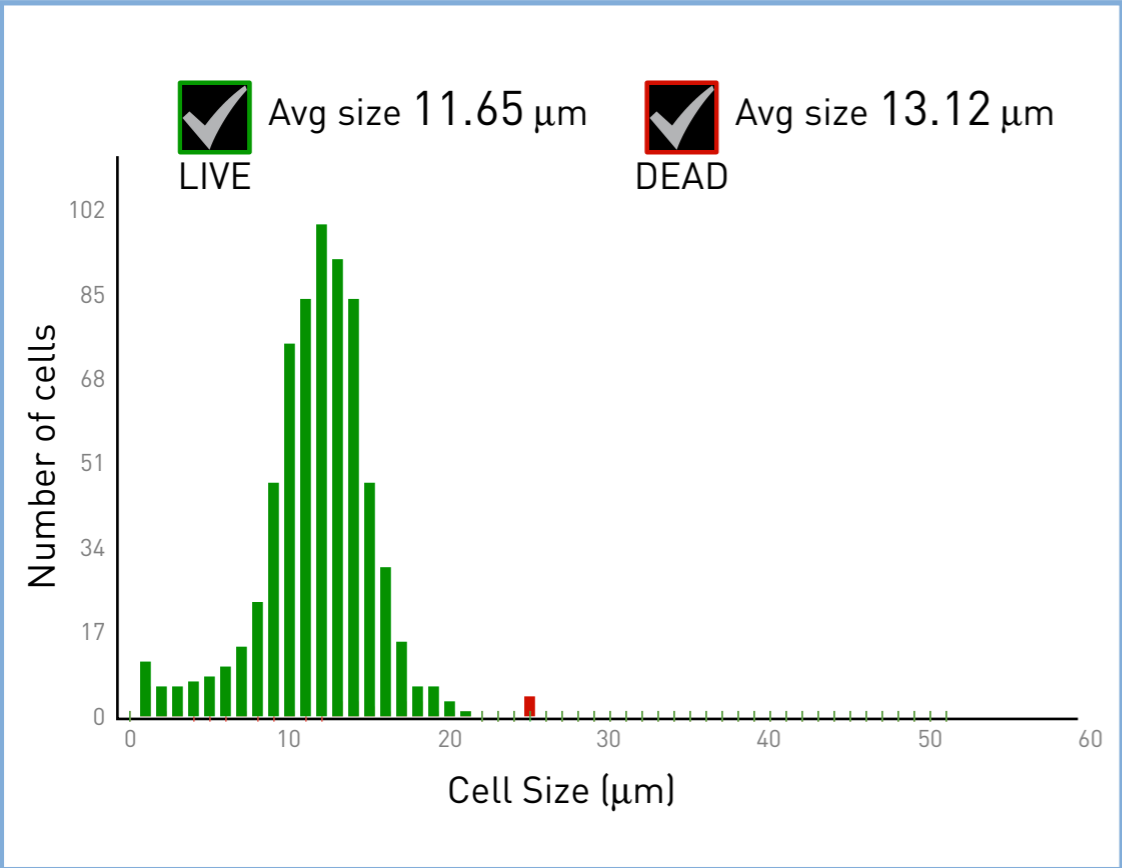

Profile: Default

Auto FL threshold: On		Live	Dead
Auto lighting: On	Size:	0 , 60	0 , 60
	Brightness:	0 , 255	0 , 255
	Circularity:	0.41	0.49