


DFN: D:\DATATY~1\OLD\04\V04\_04\V0404\_04\  
SAMPL026.D


MaxPeak: 97.13% Ret\_Time: 0.645 min

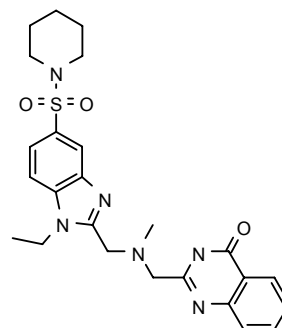


mw = 494,62

The method for the Gradient Sample using  
short rapid resolution HT Cartridge ZORBAX  
SB-C18 4.6x15 mm (p/n 821975-932). For  
testing purity of synteZ.

#	Time	Area%
1	0.600	0.80
2	0.645	97.13
3	0.707	2.07

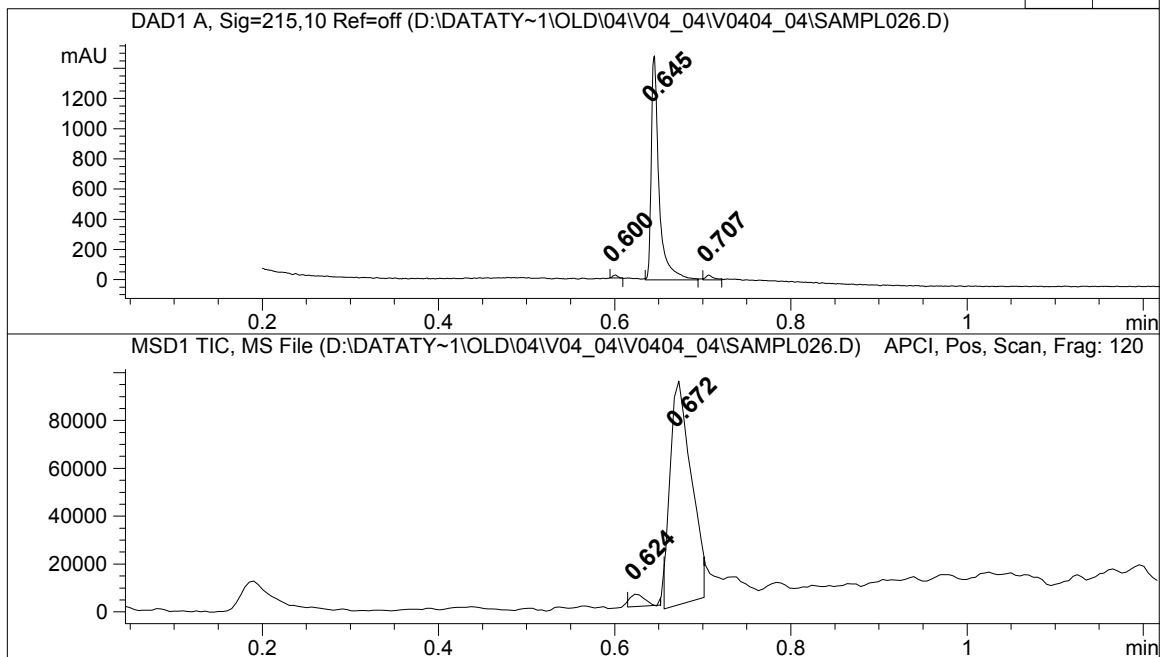

RT 0.624

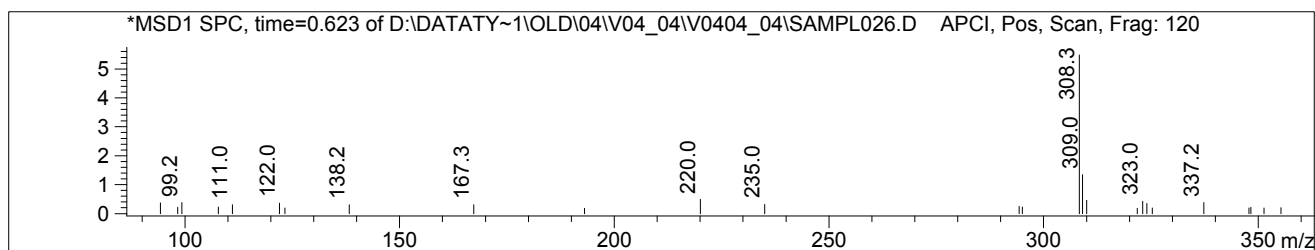

RT 0.672

