



MaxPeak: 91.76% Ret_Time: 0.751 min

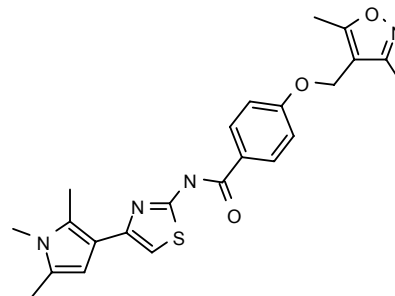


mw = 436,54

The method for the Gradient Sample using short rapid resolution HT Cartridge ZORBAX SB-C18 4.6x15 mm (p/n 821975-932). For testing purity of synteZ.


#	Time	Area%
1	0.638	5.77
2	0.751	91.76
3	0.804	2.47

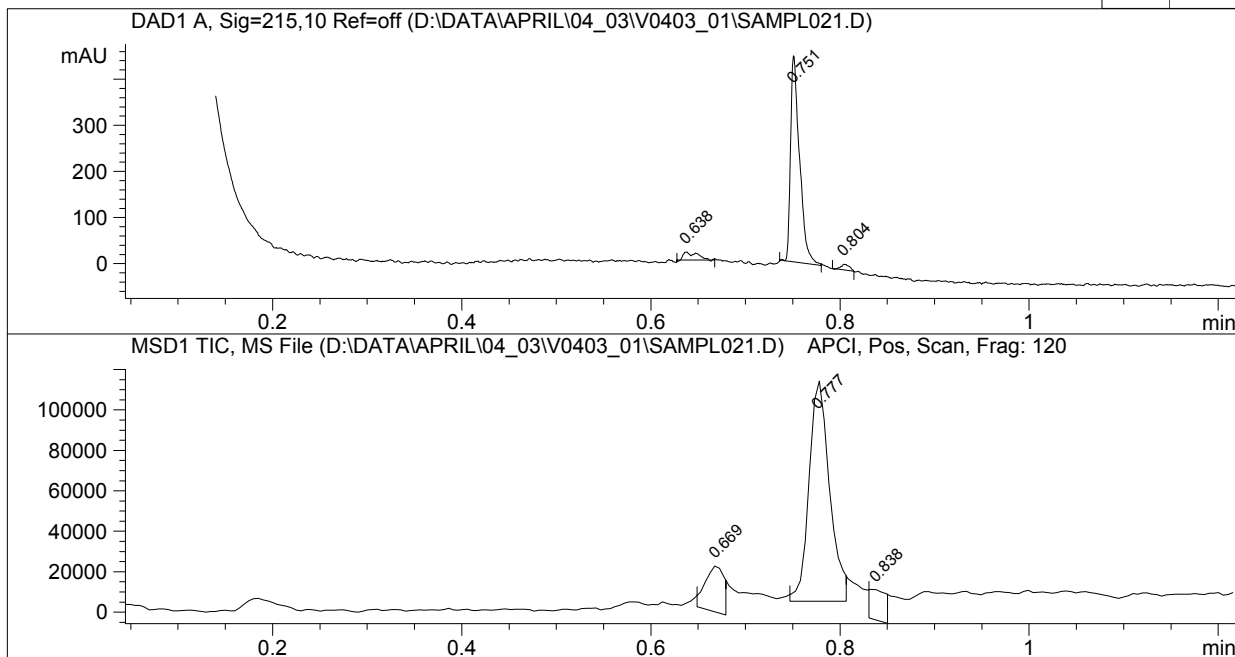

RT 0.669

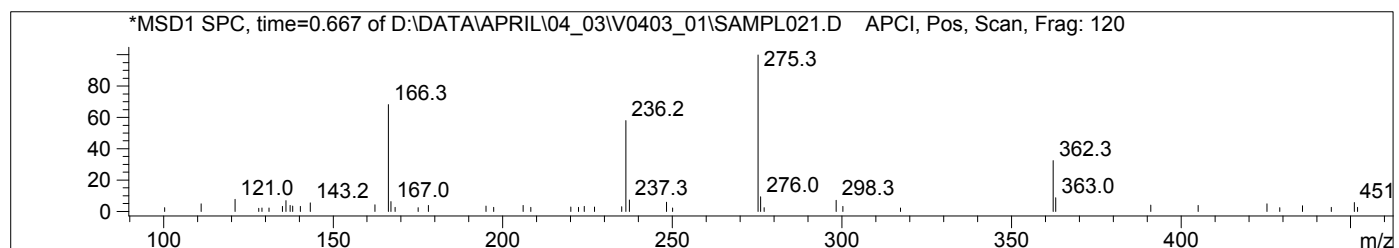

RT 0.777

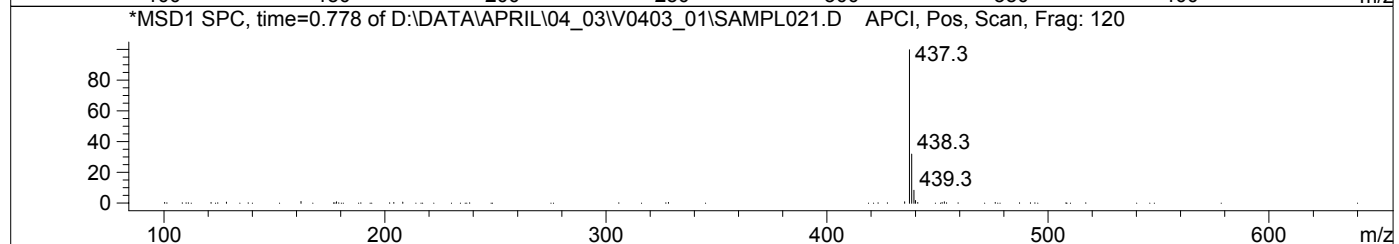

RT 0.838

