


DFN: D:\DATA~1\APRIL\04_27\04_26_06\SAMPL043.D



MaxPeak: 96.75% Ret_Time: 0.616 min

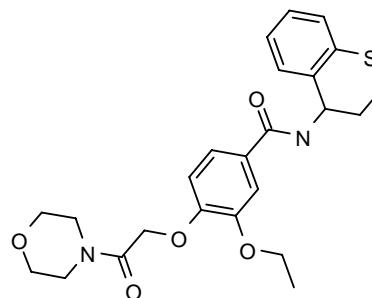

mw = 456,57

The method for the Gradient Sample using short rapid resolution HT Cartridge ZORBAX SB-C18 4.6x15 mm (p/n 821975-932). For testing purity of synteZ.

#	Time	Area%
1	0.616	96.75
2	0.691	3.25

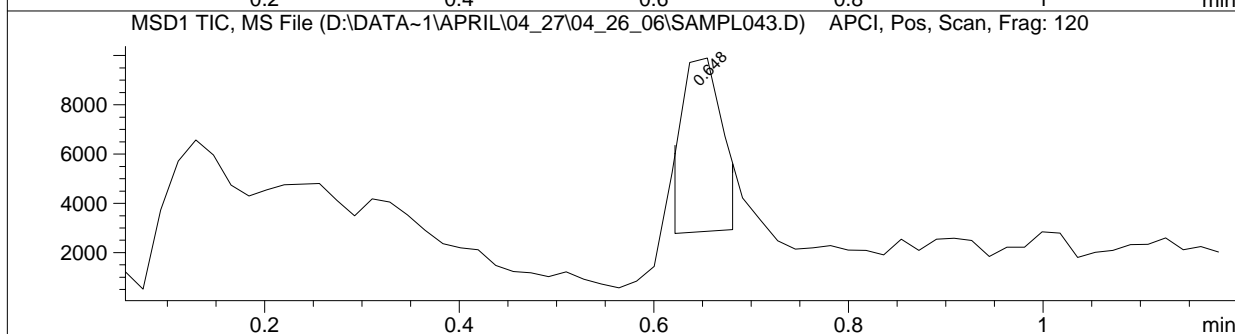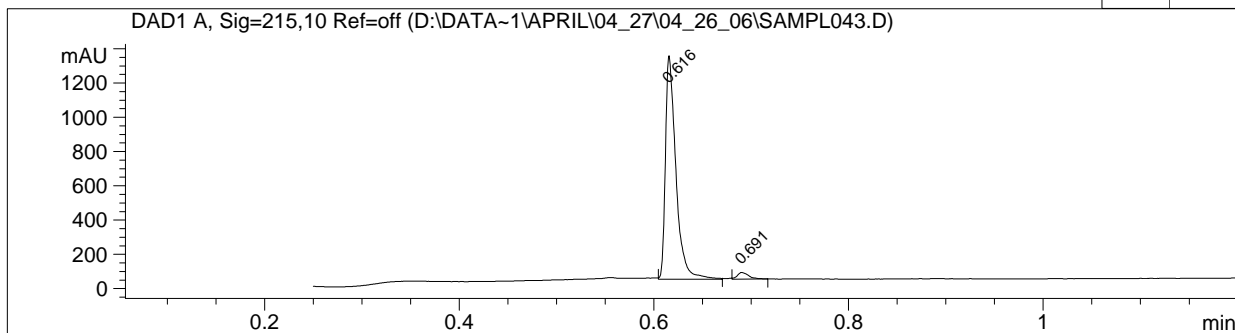

RT 0.648

