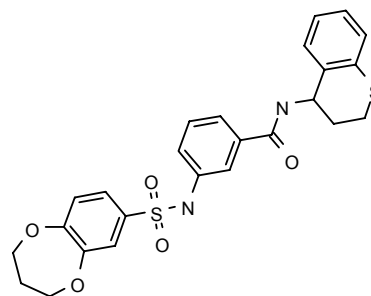


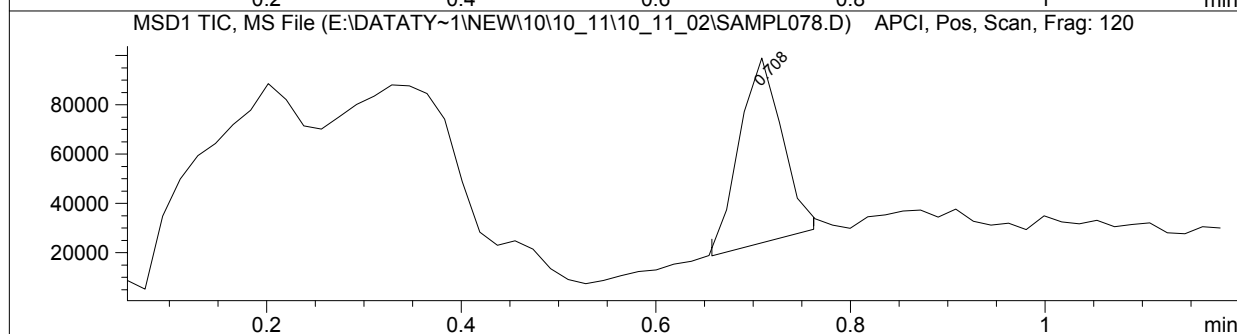
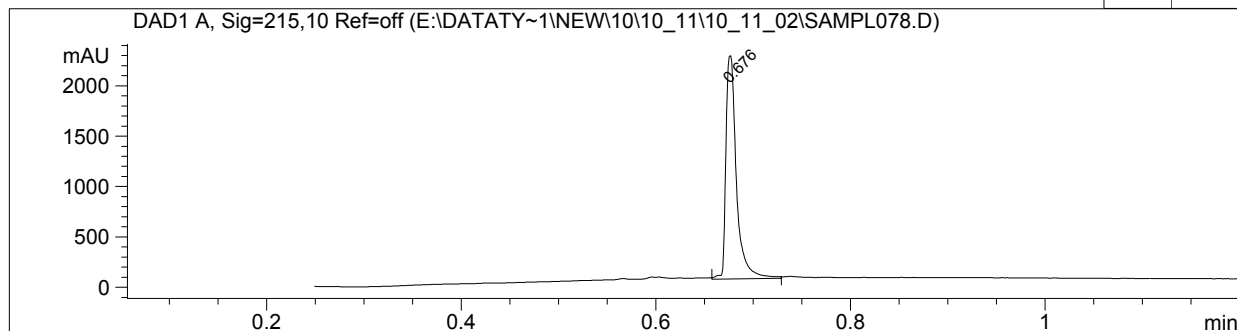
DFN: E:\DATATY~1\NEW\10\10_11\10_11_02\
SAMPL078.D-----
MaxPeak: 100.00% Ret_Time: 0.676 min

Could not execute user defined Macro ->

The method for the Gradient Sample using
short rapid resolution HT Cartridge ZORBAX
SB-C18 4.6x15 mm (p/n 821975-932). For
testing purity of synteZ.

mw = 496,61

Time Area%

1 0.676 100.00
-----

RT 0.708

