


Sample Name: 550247 OK
DFN: C:\HPCHEM\1\DATA\OLD\V04_20\V0420_09\
SAMPL028.D



MaxPeak: 91.45% Ret_Time: 0.708 min

The method for the Gradient Sample using
short rapid resolution HT Cartridge ZORBAX
SB-C18 4.6x15 mm (p/n 821975-932). For
testing purity of syntez.

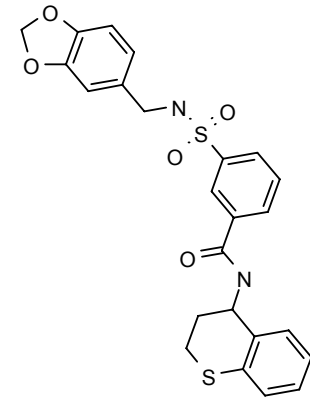

mw = 482,58

| # | Time | Area% |
|---|-------|-------|
| 1 | 0.469 | 1.14 |
| 2 | 0.535 | 2.62 |
| 3 | 0.708 | 91.45 |
| 4 | 0.763 | 4.79 |

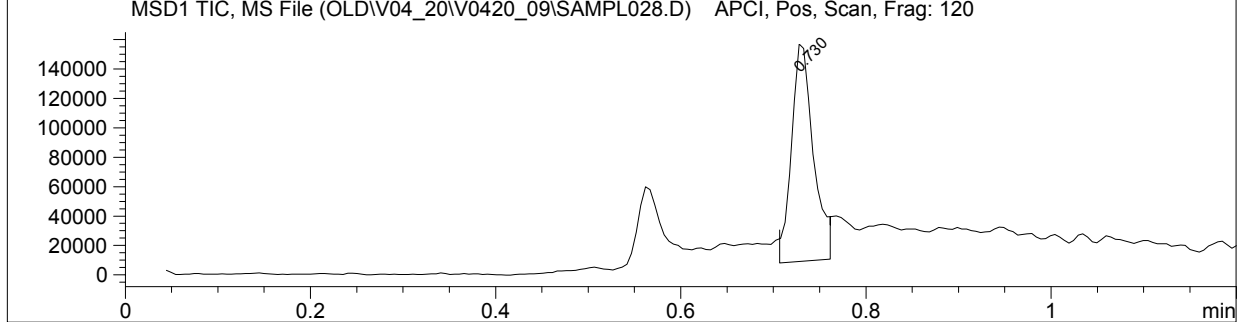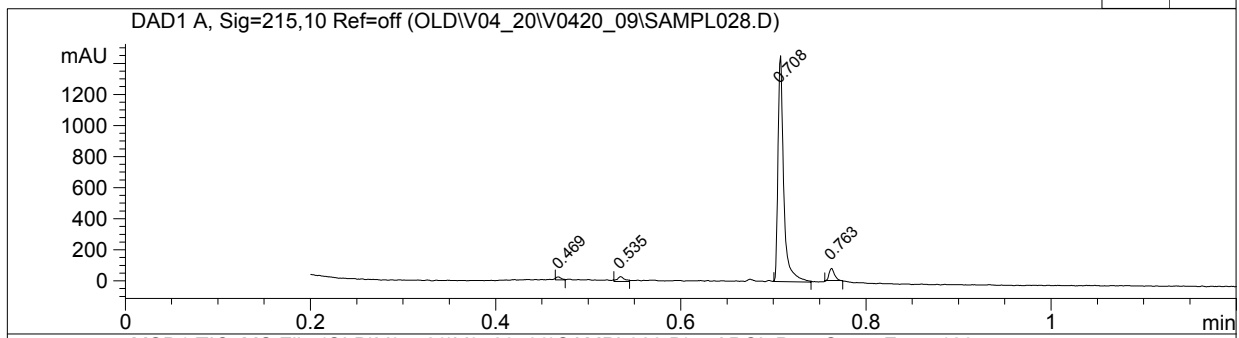

RT 0.730

