


Sample Name: 1231624

DFN: D:\DATA\MAY\05_15\V0515_02\SAMPL044.D


MaxPeak: 100.00% Ret_Time: 0.700 min

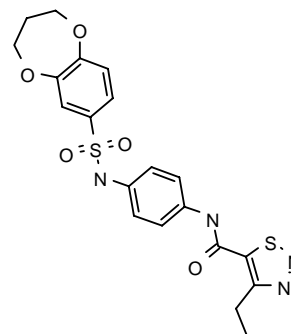

mw = 460,53

The method for the Gradient Sample using short rapid resolution HT Cartridge ZORBAX SB-C18 4.6x15 mm (p/n 821975-932). For testing purity of synte.

#	Time	Area%
1	0.700	100.00

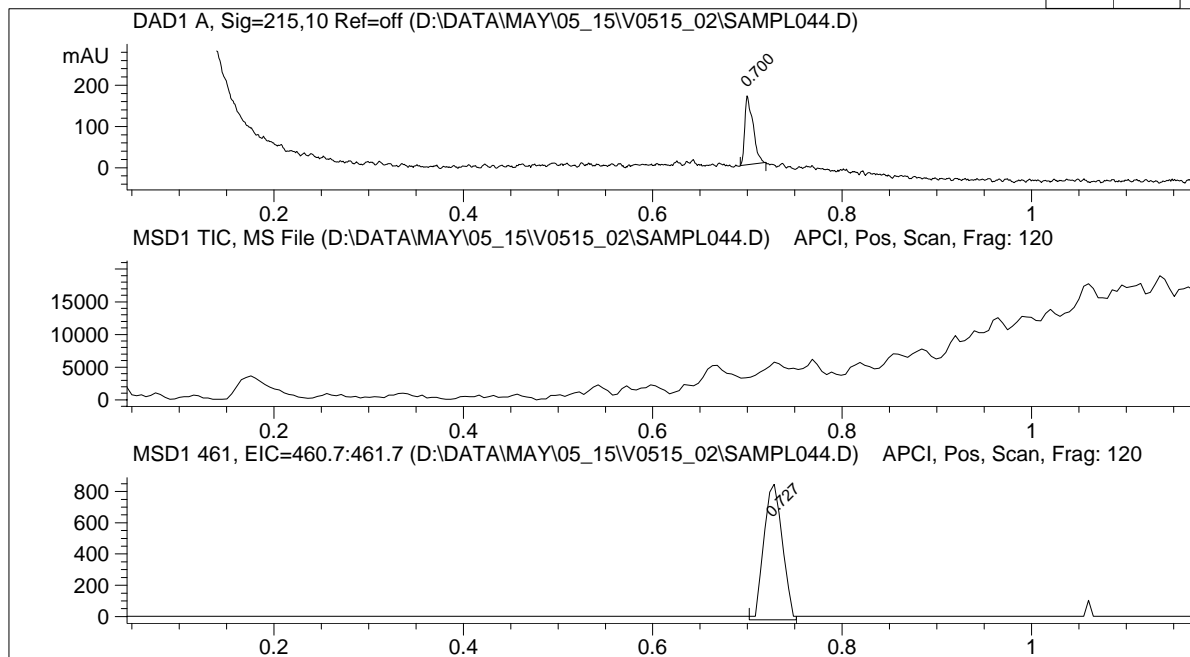

RT 0.727

