


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...-08-04\BAN300\_High Sensitivity DNA Assay\_2020-08-04\_001.xad

Created: 8/4/2020 11:44:53 AM  
Modified: 8/4/2020 12:26:12 PM

### Electrophoresis File Run Summary

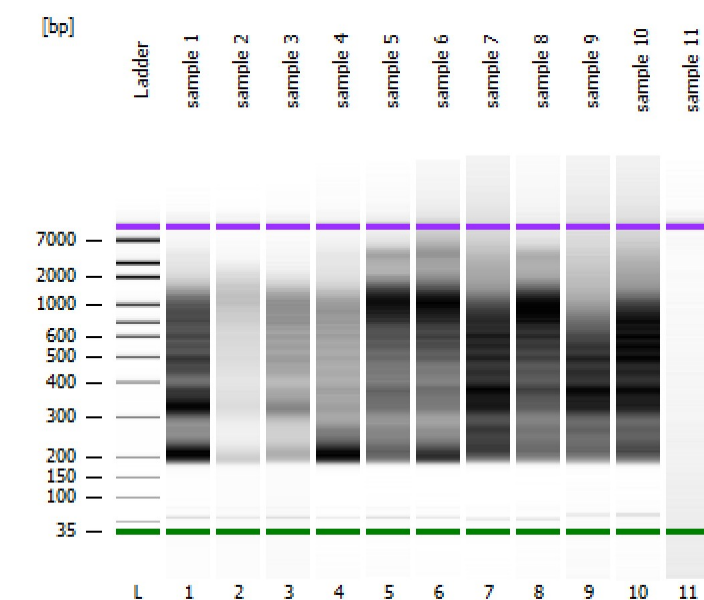

#### Instrument Information:

Instrument Name: BioA  
Serial#: DE72900930  
Firmware: C.01.069  
Type: G2939A

#### Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.0  
Assay Comments: Copyright © 2003-2009 Agilent Technologies

#### Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

