
Fig. 5; western blot

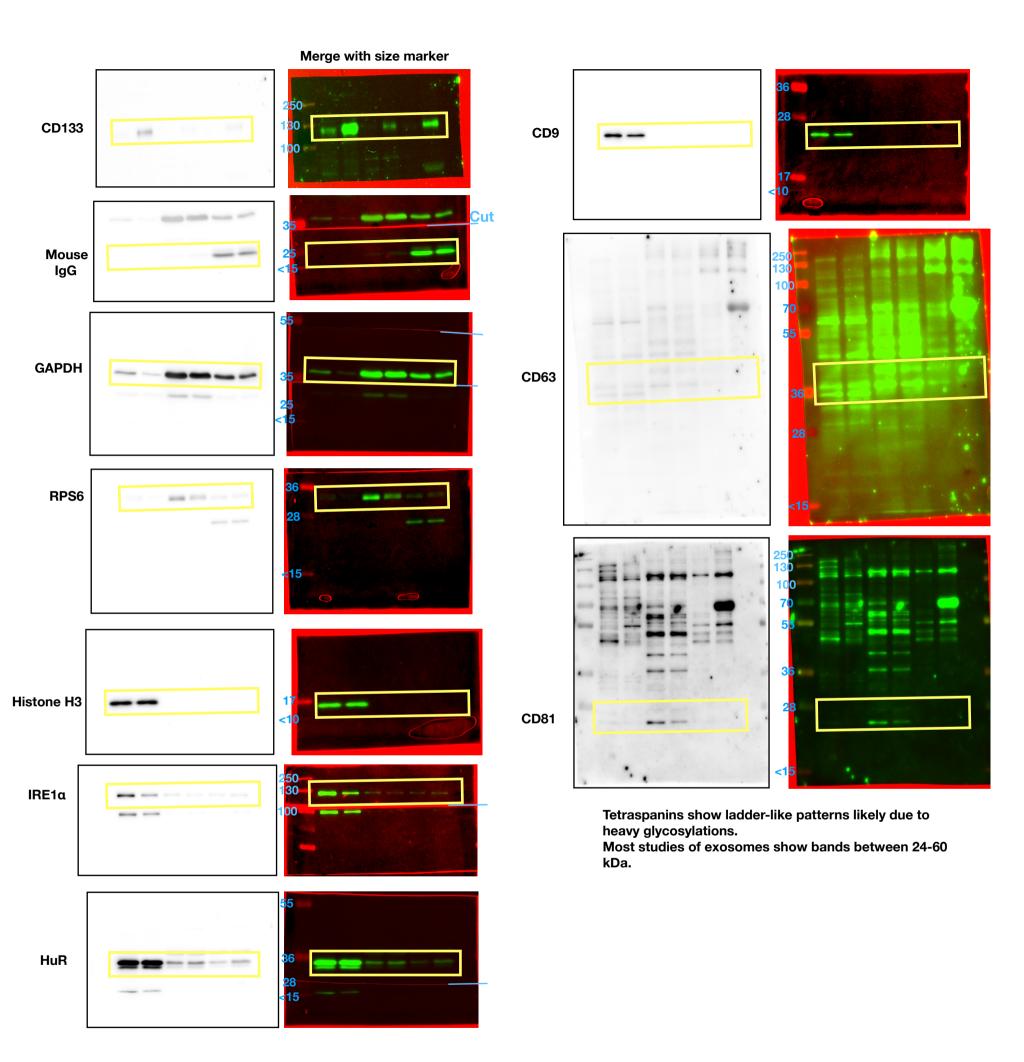

Only one linear adjustment was performed from raw data to figures (including inside the imaging instrument)